

PDF document of the Fridge-tag® 2 L

Identification number: 130500000673
 Date and time of report creation: 02.09.2016 11:15h
 Activation date: 06.06.2016 09:55h
 Upper alarm limit: Above +8.0°C for 1h
 Lower alarm limit: Below +2.0°C for 1h
 Measurement interval:¹⁾ 1min (fixed)
 Logging interval: 5min

No.	Date (dd.MM.yyyy)	Events ²⁾	Average temp.	Lower alarm limit				Upper alarm limit				Signature / notes Action taken
				Status	Min. temp.	Cumulative daily time below the limit	Alarm trigger time	Status	Max. temp.	Cumulative daily time above the limit	Alarm trigger time	
1	Today	10:29	+23.5°C	In progress	+22.5°C	0min		ALARM	+26.1°C	11h 15min	00:00h	
2	01.09.2016		+8.8°C	ok	+2.9°C	0min		ALARM	+24.1°C	5h 57min	19:03h	
3	31.08.2016		+3.6°C	ok	+3.1°C	0min		ok	+4.7°C	0min		
4	30.08.2016		+3.8°C	ok	+2.3°C	0min		ok	+8.2°C	20min		
5	29.08.2016		+3.1°C	ok	+1.9°C	14min		ok	+5.7°C	0min		
6	28.08.2016		+3.0°C	ok	+1.9°C	13min		ok	+6.0°C	0min		
7	27.08.2016		+3.1°C	ok	+1.9°C	4min		ok	+5.1°C	0min		
8	26.08.2016		+3.6°C	ok	+2.3°C	0min		ok	+7.0°C	0min		
9	25.08.2016		+3.8°C	ok	+2.3°C	0min		ok	+8.0°C	0min		
10	24.08.2016		+4.1°C	ok	+3.2°C	0min		ok	+5.7°C	0min		
11	23.08.2016		+4.1°C	ok	+3.6°C	0min		ok	+6.7°C	0min		
12	22.08.2016		+4.1°C	ok	+3.6°C	0min		ok	+5.9°C	0min		
13	21.08.2016		+3.1°C	ok	+1.8°C	27min		ok	+5.8°C	0min		
14	20.08.2016		+3.2°C	ok	+2.7°C	0min		ok	+4.5°C	0min		
15	19.08.2016		+3.1°C	ok	+1.8°C	22min		ok	+5.0°C	0min		
16	18.08.2016		+3.1°C	ALARM!	+1.5°C	1h 27min	22:18h	ok	+4.6°C	0min		
17	17.08.2016		+3.1°C	ok	+2.3°C	0min		ok	+4.1°C	0min		
18	16.08.2016		+3.2°C	ok	+2.4°C	0min		ok	+4.7°C	0min		
19	15.08.2016		+3.3°C	ok	+2.2°C	0min		ok	+5.4°C	0min		
20	14.08.2016		+2.4°C	ALARM!	+1.1°C	5h 36min	04:29h	ok	+3.7°C	0min		
21	13.08.2016		+3.3°C	ok	+2.1°C	0min		ok	+5.2°C	0min		
22	12.08.2016		+3.5°C	ok	+2.6°C	0min		ok	+4.7°C	0min		
23	11.08.2016		+3.7°C	ok	+3.0°C	0min		ok	+5.6°C	0min		
24	10.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+7.1°C	0min		
25	09.08.2016		+4.0°C	ok	+3.1°C	0min		ok	+5.1°C	0min		
26	08.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+4.9°C	0min		
27	07.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+5.0°C	0min		
28	06.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+4.8°C	0min		

1) Sampling and data analysis every minute





2) t = time / date changed, hh:mm = status checked

Date and place: _____

Signature: _____

PDF document of the Fridge-tag® 2 L

Identification number: 130500000673
Date and time of report creation: 02.09.2016 11:15h

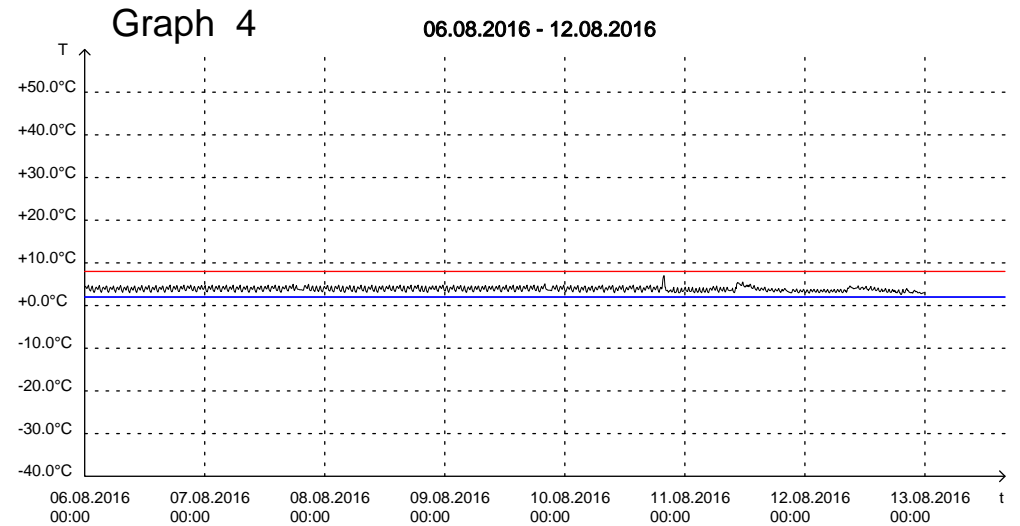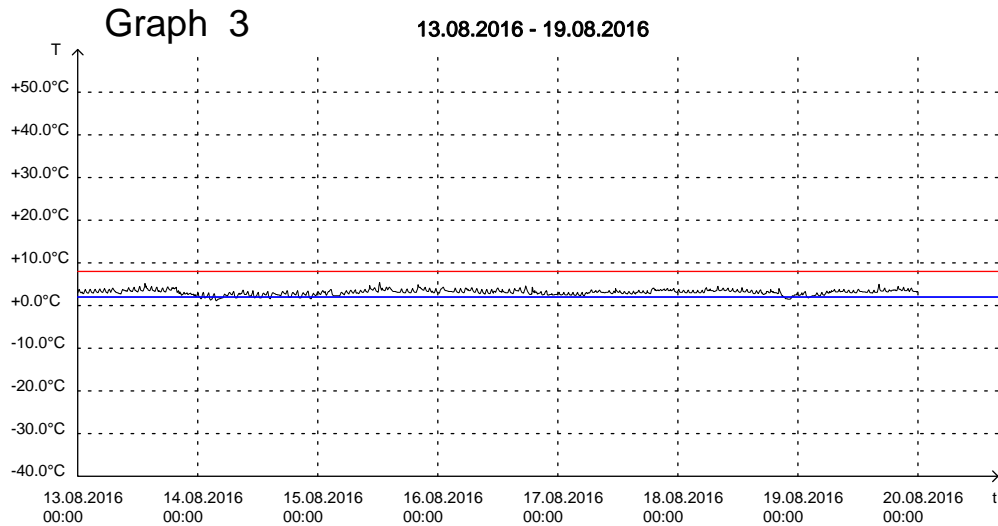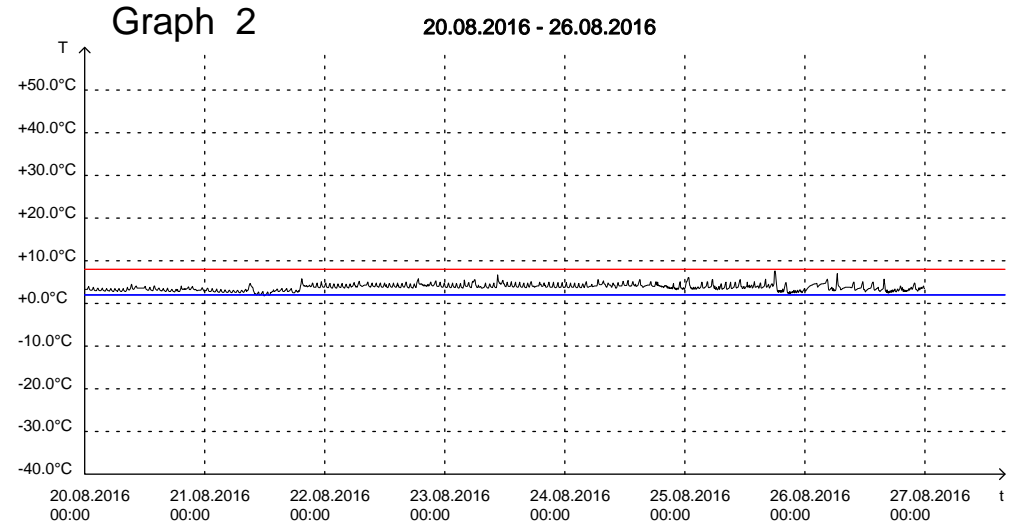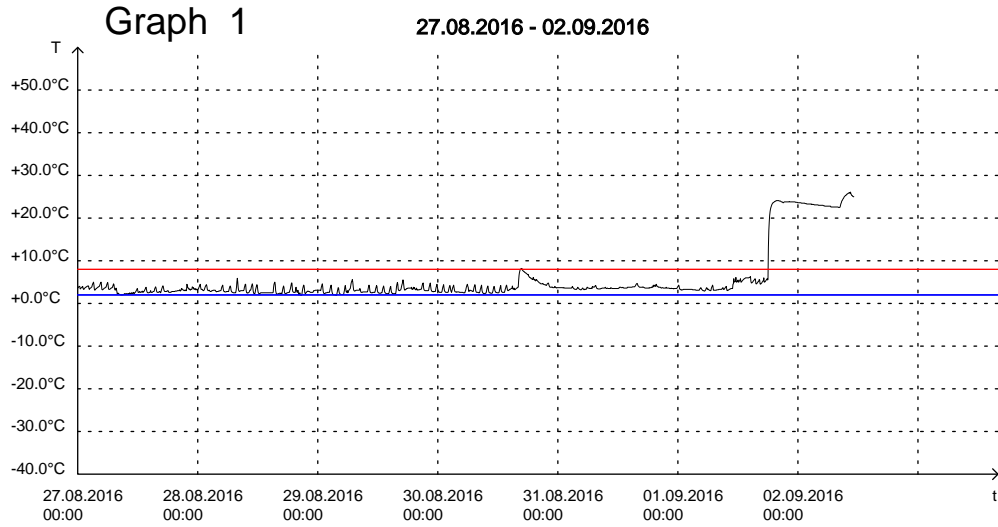

PDF document of the Fridge-tag® 2 L

Identification number: 130500000673
 Date and time of report creation: 02.09.2016 11:15h
 Activation date: 06.06.2016 09:55h
 Upper alarm limit: Above +8.0°C for 1h
 Lower alarm limit: Below +2.0°C for 1h
 Measurement interval:¹⁾ 1min (fixed)
 Logging interval: 5min

No.	Date (dd.MM.yyyy)	Events ²⁾	Average temp.	Lower alarm limit				Upper alarm limit				Signature / notes Action taken
				Status	Min. temp.	Cumulative daily time below the limit	Alarm trigger time	Status	Max. temp.	Cumulative daily time above the limit	Alarm trigger time	
29	05.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+5.3°C	0min		
30	04.08.2016		+3.8°C	ok	+2.9°C	0min		ok	+6.2°C	0min		
31	03.08.2016		+3.9°C	ok	+3.0°C	0min		ok	+6.0°C	0min		
32	02.08.2016		+4.3°C	ok	+3.3°C	0min		ok	+6.3°C	0min		
33	01.08.2016		+4.4°C	ok	+4.3°C	0min		ok	+5.0°C	0min		
34	31.07.2016		+4.5°C	ok	+4.3°C	0min		ok	+5.0°C	0min		
35	30.07.2016		+4.5°C	ok	+4.3°C	0min		ok	+5.1°C	0min		
36	29.07.2016		+4.6°C	ok	+4.5°C	0min		ok	+5.0°C	0min		
37	28.07.2016		+4.5°C	ok	+4.4°C	0min		ok	+5.0°C	0min		
38	27.07.2016		+4.6°C	ok	+4.5°C	0min		ok	+5.1°C	0min		
39	26.07.2016		+4.6°C	ok	+4.5°C	0min		ok	+5.0°C	0min		
40	25.07.2016		+5.0°C	ok	+4.6°C	0min		ok	+6.2°C	0min		
41	24.07.2016		+5.1°C	ok	+4.7°C	0min		ok	+6.5°C	0min		
42	23.07.2016		+5.4°C	ok	+4.9°C	0min		ok	+7.0°C	0min		
43	22.07.2016		+5.4°C	ok	+4.8°C	0min		ok	+6.8°C	0min		
44	21.07.2016		+5.3°C	ok	+5.0°C	0min		ok	+6.5°C	0min		
45	20.07.2016		+3.9°C	ALARM!	-0.1°C	4h 11min	00:00h	ok	+6.8°C	0min		
46	19.07.2016		+1.5°C	ALARM!	-1.7°C	13h 58min	00:52h	ok	+4.8°C	0min		
47	18.07.2016		+5.0°C	ALARM!	-0.8°C	1h 49min	23:52h	ok	+8.8°C	24min		
48	17.07.2016		+4.5°C	ok	+3.8°C	0min		ok	+6.9°C	0min		
49	16.07.2016		+4.2°C	ok	+3.8°C	0min		ok	+4.6°C	0min		
50	15.07.2016		+4.2°C	ok	+1.0°C	22min		ok	+5.3°C	0min		
51	14.07.2016		+4.4°C	ok	+4.0°C	0min		ok	+5.0°C	0min		
52	13.07.2016		+4.1°C	ok	+2.4°C	0min		ok	+5.0°C	0min		
53	12.07.2016		+4.4°C	ok	+2.3°C	0min		ok	+6.4°C	0min		
54	11.07.2016		+4.8°C	ok	+4.4°C	0min		ok	+5.7°C	0min		
55	10.07.2016		+4.9°C	ok	+4.1°C	0min		ok	+6.6°C	0min		
56	09.07.2016		+4.4°C	ok	+3.8°C	0min		ok	+5.5°C	0min		

1) Sampling and data analysis every minute

2) t = time / date changed, hh:mm = status checked

Date and place: _____

Signature: _____

PDF document of the Fridge-tag® 2 L

Identification number: 130500000673
Date and time of report creation: 02.09.2016 11:15h

